

High Speed Testing of High Brightness LEDs

Introduction

Visible light emitting diodes (LEDs) have gained a reputation for high efficiency and long lifetimes, which has led to their use in a growing list of applications, including automotive displays and exterior lights, backlighting for televisions and video monitors, street lights, outdoor signs, and interior lighting. Extensive research and development efforts by LED manufacturers have led to the creation of LEDs with higher luminous flux, longer lifetimes, greater chromaticity, and more lumens per watt, which has driven demand and encouraged an even wider array of applications. To ensure the reliability and quality of these devices, accurate and cost effective testing is critical.

LED testing involves different types of test sequences at various stages of production, such as during design research and development, on-wafer measurements during production, and final tests of packaged parts. While concrete testing “recipes” often include a multitude of steps intended to verify product lifetime or extract data on specific performance characteristics, they are beyond the scope of this application note. This note is intended to provide solid information on the needed “ingredients” for these recipes—basic tests that illustrate how to probe for the diodes’ characteristics and example test setups. This note also outlines how to achieve throughput advantages and reduce the cost of test by using new test technologies, including instruments enabled with Keithley’s Test Script Processor (TSP®).

Test Description

Testing LEDs typically involves both electrical and optical measurements. This note focuses on electrical characterization, including light measurement techniques where appropriate.

Figure 1 illustrates the electrical I-V curve of a typical diode. A complete test could include a multitude of voltage values versus current operating points, but a limited sample of points is generally sufficient to probe for the figures of merit.

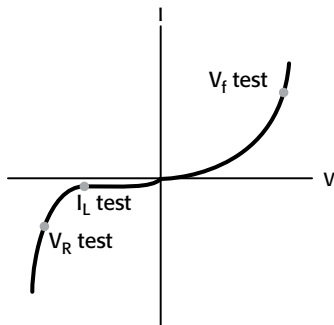


Figure 1. Typical LED DC I-V curve and test points (not to scale).

Some tests require sourcing a known current and measuring a voltage, while others require sourcing a voltage and measuring the resulting current. A SourceMeter® instrument is ideal for these types of tests because it can be configured to source voltages or currents and can also measure each of these signal types.

Forward Voltage Test (V_F) and Optical Tests

The V_F test verifies the forward operating voltage of the visible LED. When a forward current is applied to the diode, it begins to conduct. During the initial low current source values, the voltage drop across the diode increases rapidly, but the slope begins to level off as drive currents increase. The diode normally operates in this region of relatively constant voltage. It is also quite useful to test the diode under these operating conditions. The forward voltage test (V_F) is performed by sourcing a known current and measuring the resulting voltage drop across the diode. Typical test currents range from tens of milliamps to amps, while the resulting voltage measurement is typically in the range of few volts. The results of this test are typically used by manufacturers for binning purposes as the forward voltage is directly related to the chromaticity of the LED.

Forward current biasing is also used for optical tests because electrical current flow is closely related to the amount of light emitted. Optical power measurements can be made by placing a photodiode or integrating sphere close to the device under test to capture the emitted photons. This light is then converted to a current, which can be measured by an ammeter or a channel of a SourceMeter instrument.

In many test applications, the voltage and light output of the diode can be measured simultaneously using a fixed source current value. In addition, details such as spectral output can be obtained by using the same drive current value and a spectrometer.

Reverse Breakdown Voltage (V_R) and Leakage Current (I_L) Tests

Applying a negative bias current to the LED will allow probing for the so-called Reverse Breakdown Voltage (V_R). The test current should be set to a level where the measured voltage value no longer increases significantly when the current is increased slightly more. At levels higher than this voltage, large increases in reverse bias current result in insignificant changes in reverse voltage. The specification for this parameter is usually a minimum value. The test is performed by sourcing a low-level reverse bias current for a specified time, then measuring the voltage

drop across the LED. The measurement result is typically in the range of tens of volts.

Normally, moderate voltage levels (volts to tens of volts) are used to measure a Leakage Current (I_L). The Leakage Current Test measures the low-level current that leaks across the LED when a reverse voltage less than breakdown is applied. It is a common practice for leakage measurements, and more generally for isolation measurements, to make sure only that a certain threshold is not exceeded in production. There are two reasons for this. First, low current measurements require longer settling times, so they take longer to complete. Second, environmental interference and electrical noise exert greater influence on low-level signals, so extra care in shielding is required. This extra shielding complicates the test fixture and may interfere with automated handlers.

Test System Description

Single LED Test System

Figure 2 is a simplified block diagram of an LED test station. For automation purposes, a PC and a component handler—a probe station for on-wafer measurements—are included.

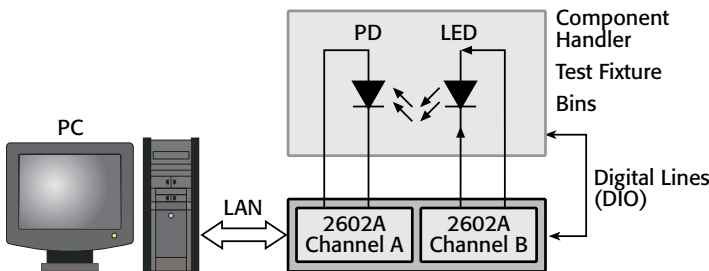


Figure 2. Block diagram of a Model 2602A SourceMeter-based single LED test system

In this system, the main purpose of the PC is to store measurement data in a database for documentation. A secondary purpose is to reconfigure the test sequence for different parts. Series 2600A instruments are unique in terms of their independence from the PC controller. Their internal Test Script Processor supports writing a complete test plan that operates on the instrument itself. In other words, a user can write a complete PASS/FAIL test sequence script and run it from the front panel of the Model 2602A without instrument reprogramming.

A more production-oriented scenario would look a bit different. In production, there may be a component handler to transport the individual LEDs to a test fixture, where they can be electrically contacted. The fixture is shielded from ambient light and houses a photodiode (PD) for light measurements. In this setup, a single Model 2602A Dual-Channel System SourceMeter instrument can be used for both connections. Source Measure Unit A (SMUA) can be used to supply the test signal to the LED and measure its electrical response while

SMUB can be used to monitor the photodiode during optical measurements.

The test sequence can be programmed to begin using a digital line from the component handler that can serve as a “start of test” (SOT) signal. After the SourceMeter instrument detects the SOT signal, the tests for characterization of the LED will begin.

After all electrical and optical tests are completed, a digital line to flag “measurement complete” can be set for the component handler. In addition, the 2602A’s built-in intelligence can perform all pass/fail operations and send a digital command through the digital I/O port on the 2602A to the component handler to bin the LED based on the pass/fail criteria. Then, usually two actions can take place synchronously: data transfer to the PC for statistical process control (SPC) and the mechanical placement of a new DUT in the testing fixture.

LED Test System for Multiple Devices/Arrays

In addition to single-device testing, there are multiple device tests, such those that involve a burn-in process. In these tests, multiple parts are measured over a specified time period. A continuous current flow is usually mandatory to drive the DUTs, but multiple light detectors may be multiplexed to a current meter by a switching system. The appropriate choices for switching system and meter will be dictated by the dynamic range of electrical currents of interest.

Keithley offers a number of switch options applicable to testing multiple LEDs. For example, the Model 3706 System Switch/Multimeter offers six slots, which can handle up to 576 multiplexed channels or 2688 matrix cross-points. It features TSP capabilities, making it the perfect companion to Series 2600A SourceMeter instruments. Through TSP-Link®, a Model 3706 and a Series 2600A SourceMeter instrument can be quickly and easily integrated. This integration allows tight synchronization of operations between the instruments and the ability to operate from a single test script, thus maximizing speed and simplicity.

For smaller numbers of LEDs, multiple Series 2600A System SourceMeter instruments can be used. **Figure 3** illustrates a three-LED device test system with one PD channel.

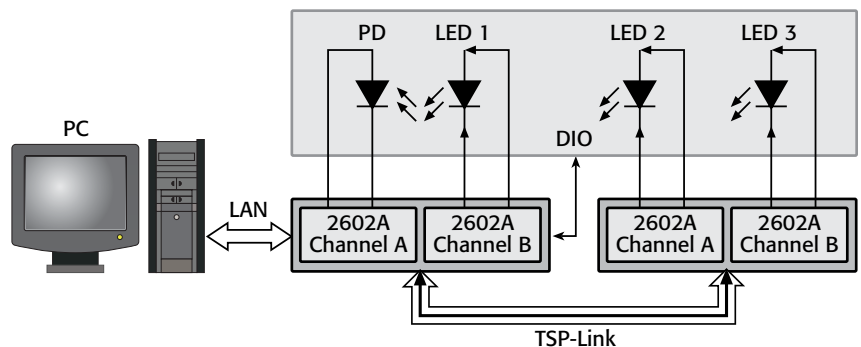


Figure 3. Block diagram with scalable Model 2602A SourceMeter channels for an LED array test system

Test Sequence Script Code

The following code snippets illustrate a test sequence script for the Model 2602A to perform three simple electrical tests on an LED. The intention of the test steps are to serve as building blocks for creating more specialized applications.

The first part after the enumeration of tests is a one-time-only configuration, providing a well-defined starting condition of the instrument. Next, the output of the SMU channel is activated and the tests follow sequentially. The measurement data is stored in the variable "Reading" and is sent to a PC via "print" commands at the end of the listing.

Note: double hyphens (--) indicate comment lines.

First, let's put the instrument into a default setting by sending the following function:

```
-- Example LED Test Sequence -- 1.) Forward Voltage Test VF at 10 mA
-- 2.) Leakage Current Test IL at -10 V
-- 3.) Reverse Breakdown Voltage Test VR at -5E-6 A

function ResetLED()
-- One Time Reset & Setup
Reading = {} --Create table for readings
smua.reset() --reset SMU
smua.measure.nplc = 0.01 --Set measurement aperture
smua.measure.autozero = smua.AUTOZERO_OFF --Disable autozero
smua.sense = smua.SENSE_REMOTE --Enable 4-wire measurement
--GlobalVar = 1
end--function ResetLED()
```

To perform the test sequence, we need another function that sets up each test and performs the proper actions:

```
function LEDTest()
--configure LED Test Sequence.
--Performs VF, IL, and VR tests

smua.source.levelv = 0 --Set source value
smua.source.output = smua.OUTPUT_ON --Enable source

--1.) Forward Voltage Test VF at 10 mA
smua.measure.rangev = 6 --Set measurement range
smua.source.limiti = 0.001 --Set source current compliance
smua.source.rangei = 0.1 --Set source range
smua.source.leveli = 0.01 --Set source level
--Select output function
smua.source.func = smua.OUTPUT_DCAMPS
smua.source.limitiv = 6 --Set source voltage compliance
delay (0.001) --Delay
Reading[1] = smua.measure.v() --Perform Vf measurement

--2.) Leakage Current Test IL at -10 V
--Select current measurement range
smua.measure.rangei = 1E-5smua.source.rangev = 40 --Select voltage source range
smua.source.levelv = -10 --Select voltage source value
--Set source function
smua.source.func = smua.OUTPUT_DCVOLTS smua.source.limiti = 0.1 --Set source current compliance
delay (0.005) --Delay
Reading[2] = smua.measure.i() --Perform IL measurement

--3.) Reverse Breakdown Voltage Test VR at -5E-6 A
smua.measure.rangev = 40 --Set voltage measurement range
smua.source.rangei = 1E-5 --Set current source range
smua.source.leveli = -5E-6 --Set current source level
smua.source.limitiv = 40 --Set source voltage compliance
smua.source.func = smua.OUTPUT_DCAMPS --Set source function
delay (0.005) --Delay
Reading[3] = smua.measure.v() --Perform VR measurement

smua.source.leveli = 0 --Set source level
smua.source.output = smua.OUTPUT_OFF --Disable output

end--function LEDTest()
```

And finally, we need to return the data to the computer:

```
function ReturnData()  
  
-- Data Printing  
print ("")  
print ("Measurement reading at 10 mA:".. Reading[1].." V")  
print ("Measurement reading at -10 V:".. Reading[2].." A")  
print ("Measurement reading at -5 uA:".. Reading[3].." V")  
  
end --function ReturnData()
```

These functions can now be called by an external program, such as Visual Basic® or LabVIEW®, simply by sending the string of the function name.

Here is an example for a system using VB6 Control via Ethernet:

NOTE: The single quote (') denotes a comment in Visual Basic® 6.

```
Call Send(KeithleyMeter, "ResetLED()", status) 'Calls ResetLED()  
  
Call Send(KeithleyMeter, "LEDTest()", status) 'Calls LEDTest()  
  
'Calls ReturnData()  
Call Send(KeithleyMeter, "ReturnData()", status)
```

We now need to enter the data to our external program:

```
For I = 1,4  
--There are 4 print statements.. so we need 4 enters  
Call enter(Data, 1000, Length, KeithleyMeter, status) ' Get info back from meter  
Data = Data & Data 'Concatenate data string  
Loop
```

This will return the characters that are held in the output buffer queue in the order they were written. The data returned in this case was ASCII. This is not the fastest method of data return, but it is the easiest to start with. Consult the software program and instrument manuals for directions on more expedient data transfer techniques, such as binary data transfer and buffered data storage.

Programming Tests for Speed: TSP

With many instruments, the PC controls all aspects of the test. In each element of a test sequence, the instruments must be configured for each test, perform the desired action, and then return the data to the controlling PC (*Figure 4*). The controlling PC then must evaluate the pass/fail criteria and perform the appropriate action for binning the DUT. Each command sent and executed consumes precious production time and lowers throughput.

Obviously, a large percentage of this test sequence time is consumed by communicating information to and from the PC. Series 2600A instruments offer the unique ability to increase the throughput of complicated test sequences dramatically by decreasing the amount of traffic over the communications bus. In these instruments, the majority of the test sequence is embedded in the instrument. The Test Script Processor (TSP) is a full-featured test sequence engine that allows control of the test sequence, with internal pass/fail criteria, math, calculations, and control of digital I/O (see the Test Sequence with 2602A illustrated in *Figure 5*). The TSP can store a user-defined test sequence in memory and execute it on command. This limits the set-up

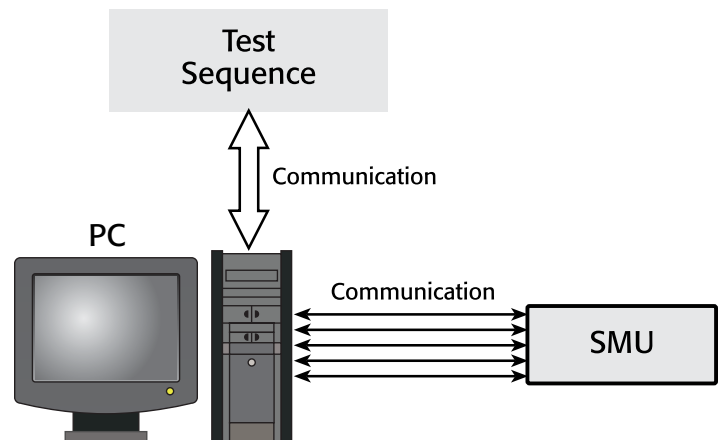


Figure 4. PC control of standard instruments.

and configuration time for each step in the test sequence and increases throughput by lessening the amount of communications to and from the instrument and PC.

Here is a simple step-by-step process for programming the Model 2602A:

- 1) Create the script.

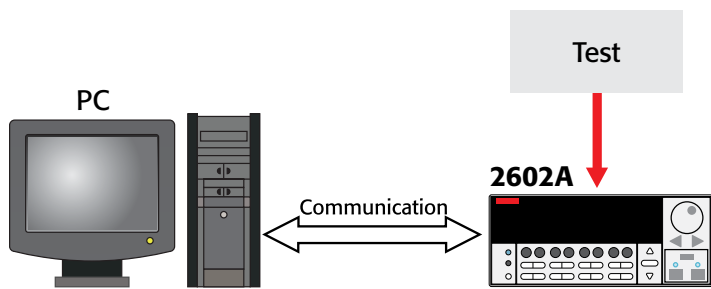


Figure 5. Use of the embedded Test Script Processor (TSP) in the Model 2602A to store the test sequence. Note decreased communications traffic.

- 2) Download the script to the instrument.
- 3) Call the script to run.

The 2602A script can be written in the Test Script Builder software provided with the instrument or downloaded to the instrument using another program, such as Visual Basic or LabVIEW. See Section 2 of the Series 2600A User's Manual for more information on programming the 2602A.

Typical Sources of Error

Junction Self-Heating

With increasing test times, the semiconductor junction of the LED will tend to heat. The two tests susceptible to junction heating are the forward voltage and leakage current tests. As the junction heats, the voltage will drop or, more importantly, the leakage current will increase during the constant voltage test. Therefore, it is important to shorten the test time as much as possible without sacrificing measurement accuracy or stability.

The Series 2600A System SourceMeter family can configure the device soak time before the measurement, as well as the amount of time the input signal is acquired. The soak time allows any circuit capacitance to settle before the measurement begins. The measurement integration time is determined by the number of power line cycles (NPLC). If the input power were at 60Hz, a 1NPLC measurement would require 1/60th of a second or 16.667ms. The integration time defines how long the analog-to-digital converter (ADC) acquires the input signal, and it represents a trade-off between speed and accuracy.

Typical soak times for the V_F test are from less than a few hundred microseconds to five milliseconds, and from five to 20 milliseconds for the I_L test. By using these short test times, errors due to the junction heating are reduced. Also, the junction heating characteristics can be determined by performing a series of tests and only varying the test time.

To further aid in test time reduction and thus junction self-heating, the Series 2600A SourceMeter instruments are also capable of pulsed operation. In this mode, they are able to source their outputs precisely for a specified duration of time. Pulse width resolution of one microsecond gives precise control over how long power is applied to the device and 500 nanosecond pulse width accuracy ensures that measurements are repeatable. Pulsed operation also gives the Series 2600A SourceMeter instru-

ments the ability to output current levels well beyond the DC capabilities of the instrument. For example, the 2602A can output 3 amps DC at 6 volts. In pulsed mode, it is capable of outputting 10 amps at 20 volts. This makes Series 2600A SourceMeter instruments an excellent choice not only now, but for the future as device current requirements increase.

Lead Resistance

A common source of voltage measurement error is the series resistance from the test leads running from the instrument to the LED. This series resistance is added into the measurement when making a two-wire connection (see *Figures 6 and 8*). The effects of lead resistance are particularly detrimental when long connecting cables and high currents are used, because the voltage drop across the lead resistance becomes significant compared to the measured voltage.

Figure 8 depicts the situation with lead resistances drawn as 'lumped' components. The gray "rounded rectangle" sketches current flow, which is nearly unaffected by high impedance voltage meters.

To eliminate this problem, use the four-wire remote sensing method, rather than the two-wire technique. With the four-wire method (see *Figures 7 and 9*), a current is forced through the LED using the Output HI/LO test leads, and the voltage across the LED is measured using the Sense HI/LO set of leads. As a result, only the voltage drop across the LED is measured.

Leakage Current

Stray leakage in cables and fixtures can be a source of error in measurements involving very low currents, such as for leakage currents. To minimize this problem, construct test fixturing with high resistance materials. Another way to reduce leakage currents is to use the built-in guard of the SourceMeter instrument. The guard is a low impedance point in the circuit that has nearly the same potential as the high impedance point to be guarded.

This concept is best illustrated by example (*Figure 10*). In this example, the LED to be measured is mounted on two insulated standoffs. Guarding is used in this circuit to ensure that all the current flows through the diode and not through the standoffs. In general, guarding should be used when sourcing or measuring currents less than $1\mu\text{A}$. Connecting the Guard terminal of the instrument to the metal guard plate guards this circuit. This puts the bottom of the DUT insulator standoffs at almost the same potential as the top. Both ends of the insulator are at nearly the same potential, so no significant current can flow through it. All the current will then flow through the LED as desired.

WARNING: Guard is at the same potential as Output HI. Therefore, if hazardous voltages are present at output HI, they are also present at the Guard terminal.

Electrostatic Interference

High resistance measurements can be affected by electrostatic interference, which occurs when an electrically charged object is brought near an uncharged object. To reduce the effect of elec-

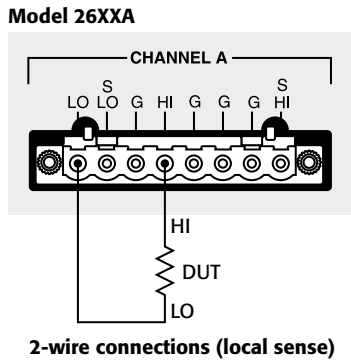


Figure 6. Two-wire connections to a 260XA SourceMeter channel.

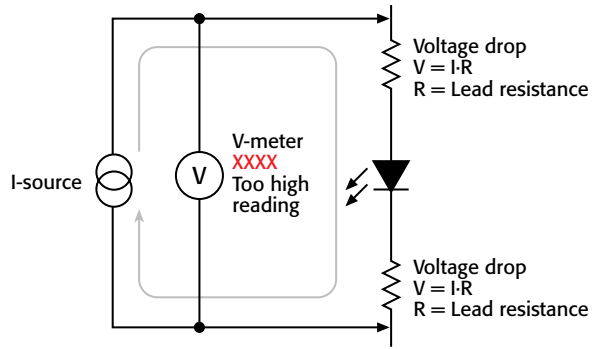


Figure 8. Two-wire connections to an LED.

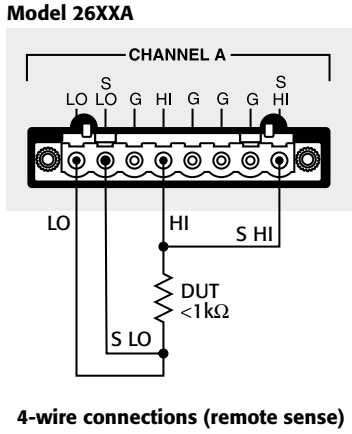


Figure 7. Four-wire connections to a 260XA SourceMeter channel.

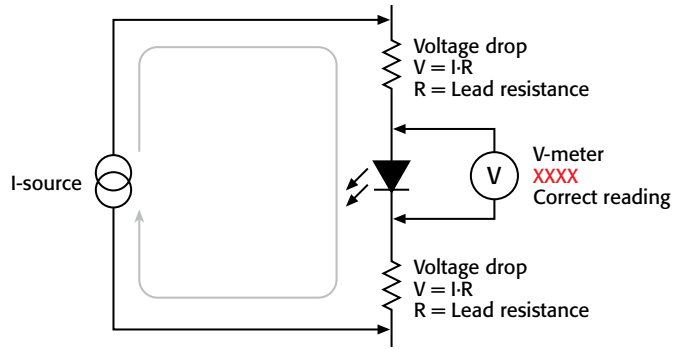


Figure 9. Four-wire connections to an LED.

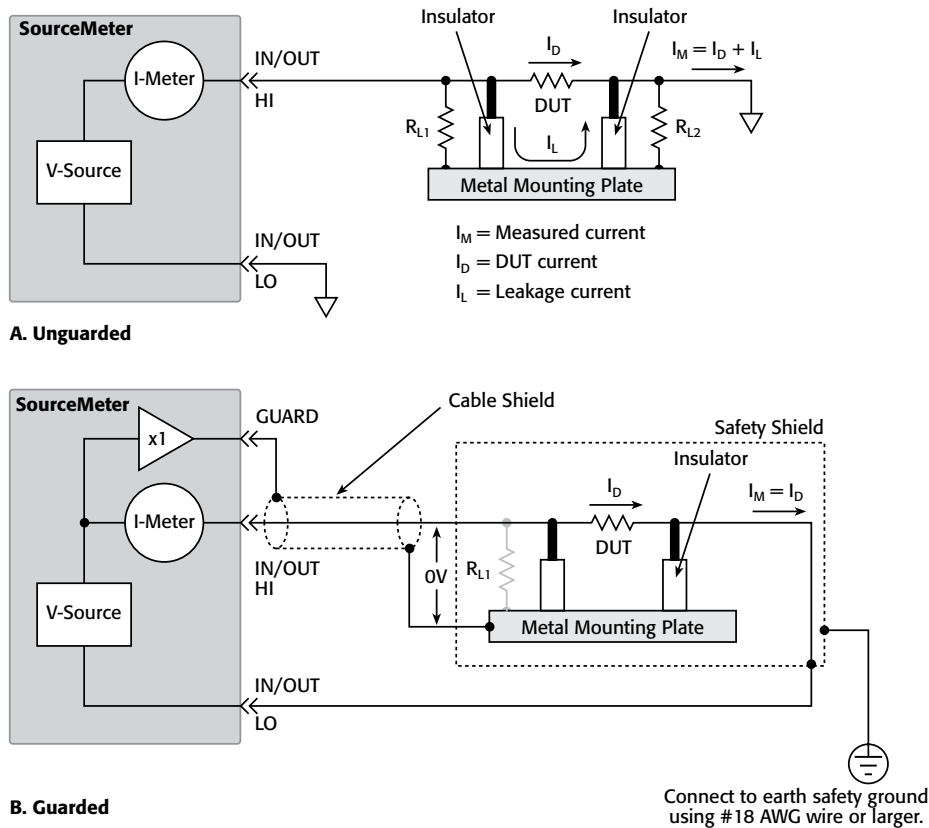


Figure 10. Comparison of unguarded and guarded measurements.

trostatic fields, a shield can be built to enclose the circuit being measured. As shown in *Figure 10B*, a metal shield connected to ground surrounds the LED under test. The Output LO terminal of the SourceMeter instrument must be connected to the metal shield to avoid noise due to common mode and other interference. Using this type of shield will also help shield operators from contacting the standoff metal plate, because the plate is at guard potential.

Light Interference

Testing LEDs involves detecting the amount and intensity of light produced by the LED, so the test fixture should be shielded from light. Typically, the inside of a test fixture is painted black in order to reduce reflection within the fixture.

Equipment List

The following equipment is needed to configure the system shown in *Figure 2*:

- Model 2602A System SourceMeter instrument.
- PC with Ethernet port and cable.
- Light-shielded enclosure with calibrated photodetector.
- Custom digital I/O cable for connecting the 25-pin male D-sub connector of the SourceMeter to the component handler.
- Custom wiring harness for connecting the test equipment to the DUT and photodetector.

One additional Model 2602A and one TSP-Link cable are needed to configure the system shown in *Figure 3*.

Test System Safety

Many electrical test systems or instruments are capable of measuring or sourcing hazardous voltage and power levels. It is also possible, under single fault conditions (e.g., a programming error or an instrument failure), to output hazardous levels even when the system indicates no hazard is present.

These high voltage and power levels make it essential to protect operators from any of these hazards at all times. Protection methods include:

- Design test fixtures to prevent operator contact with any hazardous circuit.
- Make sure the device under test is fully enclosed to protect the operator from any flying debris. For example, capacitors and semiconductor devices can explode if too much voltage or power is applied.
- Double insulate all electrical connections that an operator could touch. Double insulation ensures the operator is still protected, even if one insulation layer fails.
- Use high reliability, fail-safe interlock switches to disconnect power sources when a test fixture cover is opened.
- Where possible, use automated handlers so operators do not require access to the inside of the test fixture or have a need to open guards.
- Provide proper training to all users of the system so they understand all potential hazards and know how to protect themselves from injury. It is the responsibility of the test system designers, integrators, and installers to make sure operator and maintenance personnel protection is in place and effective. Specifications are subject to change without notice.

For More Information:



Leading the way in test and measurement

Vicom Australia

1064 Centre Rd
Oakleigh South Vic
3167 Australia 1300
360 251
info@vicom.com.au
www.vicom.com.au

Vicom New Zealand

Grd Floor, 60 Grafton Road
Auckland 1010
New Zealand
+64 9 379 4596
info@vicom.co.nz
www.vicom.co.nz

Specifications are subject to change without notice.
All Keithley trademarks and trade names are the property of Keithley Instruments, Inc.
All other trademarks and trade names are the property of their respective companies.



A G R E A T E R M E A S U R E O F C O N F I D E N C E

KEITHLEY INSTRUMENTS, INC. ■ 28775 AURORA RD. ■ CLEVELAND, OH 44139-1891 ■ 440-248-0400 ■ Fax: 440-248-6168 ■ 1-888-KEITHLEY ■ www.keithley.com

BELGIUM

Sint-Pieters-Leeuw
Ph: 02-3630040
Fax: 02-3630064
info@keithley.nl
www.keithley.nl

CHINA

Beijing
Ph: 86-10-8447-5556
Fax: 86-10-8225-5018
china@keithley.com
www.keithley.com.cn

FRANCE

Saint-Aubin
Ph: 01-64532020
Fax: 01-60117726
info@keithley.fr
www.keithley.fr

GERMANY

Germering
Ph: 089-84930740
Fax: 089-84930734
info@keithley.de
www.keithley.de

INDIA

Bangalore
Ph: 080-26771071, -72, -73
Fax: 080-26771076
support_india@keithley.com
www.keithley.com

ITALY

Peschiera Borromeo (Mi)
Ph: 02-5538421
Fax: 02-55384228
info@keithley.it
www.keithley.it

JAPAN

Tokyo
Ph: 81-3-5733-7555
Fax: 81-3-5733-7556
info.jp@keithley.com
www.keithley.jp

KOREA

Seoul
Ph: 82-2-574-7778
Fax: 82-2-574-7838
keithley@keithley.co.kr
www.keithley.co.kr

MALAYSIA

Penang
Ph: 60-4-643-9679
Fax: 60-4-643-3794
koh_william@keithley.com
www.keithley.com

NETHERLANDS

Gorinchem
Ph: 0183-635333
Fax: 0183-630821
info@keithley.nl
www.keithley.nl

SINGAPORE

Singapore
Ph: 65-6747-9077
Fax: 65-6747-2991
koh_william@keithley.com
www.keithley.com

SWITZERLAND

Zürich
Ph: 044-8219444
Fax: 044-8203081
info@keithley.ch
www.keithley.ch

TAIWAN

Hsinchu
Ph: 886-3-572-9077
Fax: 886-3-572-9031
info_tw@keithley.com
www.keithley.com.tw

UNITED KINGDOM

Theale
Ph: 0118-9297500
Fax: 0118-9297519
info@keithley.co.uk
www.keithley.co.uk